Biosim Peptides

Project 135557
Lab # 131049
Date Rec'd 12/9/2025
Report Issued 12/12/2025

Project
Sample KLOW 80

Certificate of Analysis



Analyte	Result	LOQ	Units	% of Label	Method	Date	CAS
Peptide Analysis							
Chromatographic purity	98.99	0.5	%		HPLC-UV/MS	12/9/2025	
BPC-157	10.5	0.5	mg	105.5	HPLC-UV-MS	12/9/2025	137525-51-0
BPC-157	ID Confirmed	0.5	mg		HPLC-UV-MS	12/9/2025	
GHK-Cu	50.6	0.5	mg	101.1	HPLC-UV-MS	12/9/2025	49557-75-7
GHK-Cu	ID Confirmed	0.5	mg		HPLC-UV-MS	12/9/2025	
KPV	9.29			92.9	HPLC-UV-MS	12/9/2025	112965-21-6
KPV	ID Confirmed				HPLC-UV-MS	12/9/2025	
Thymosin β4	9.83			98.3	HPLC-UV-MS	12/9/2025	77591-33-4
Thymosin β4	ID Confirmed				HPLC-UV-MS	12/9/2025	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
Methods shown reference current Krause Analytical SOPs


ND - Not detected LOQ - limit of quantification

Copyright © 2025 Krause Analytical LLC. All rights reserved.

Respectfully submitted,

Mark C. Krause
Laboratory Director

Chromatogram

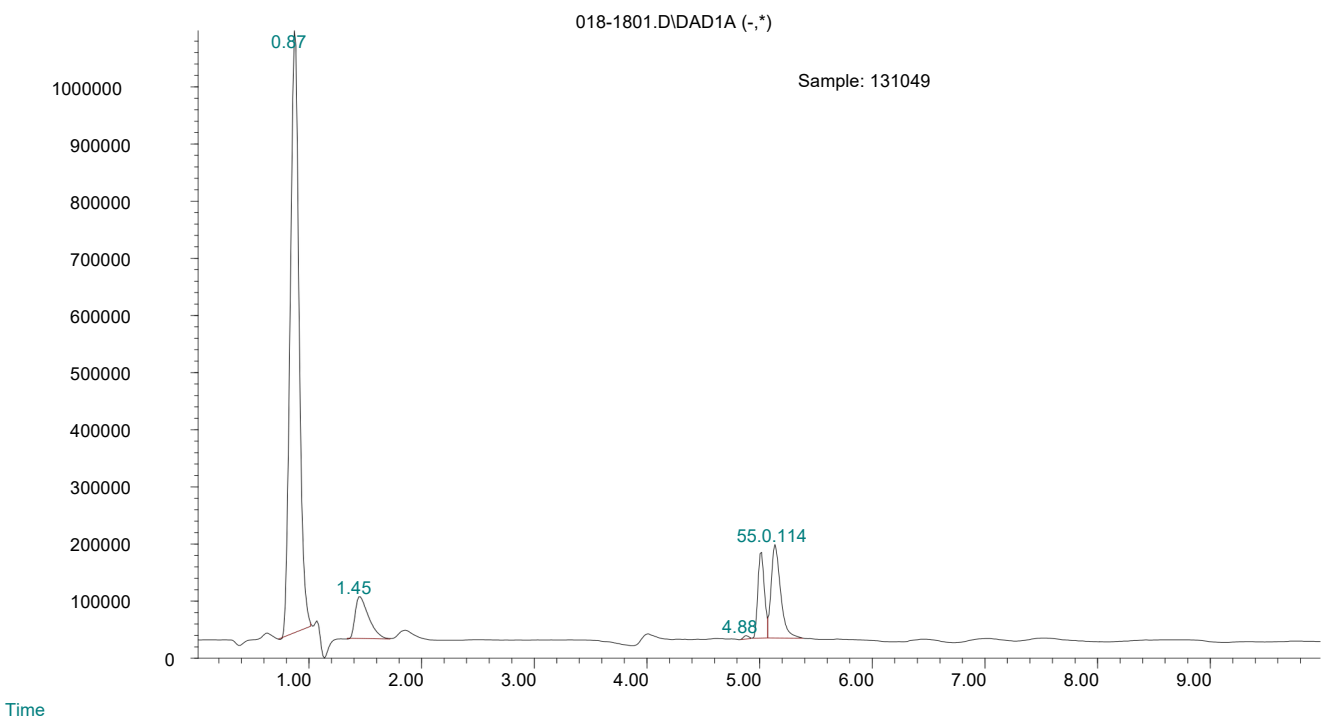

Mass spectrum/Reference Spectrum

